

Supplemental information

¹Debdutt Patro, ¹Sravan Josyula, ¹Harish P, ²Fabio Alemano and ²Deepak Halenahally Veeregowda

Global Application Team, ¹Ducom Instruments, India, ²Ducom Instruments, Netherlands

a

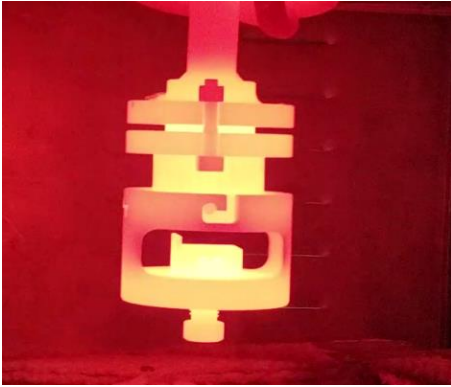


Figure 1. 1000 °C sample mounted in erosion holder

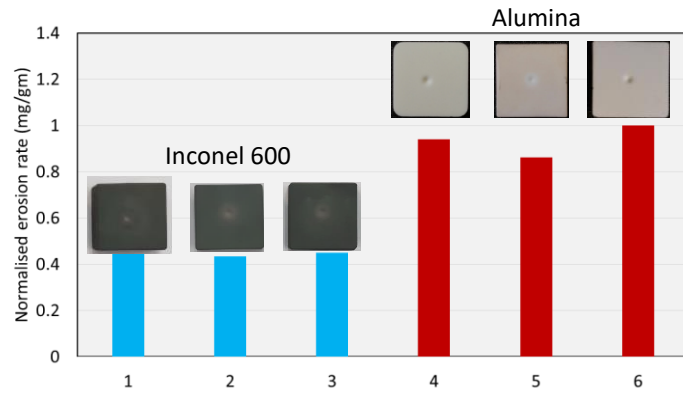


Figure 2. 1000 °C erosion rates for IN600 and alumina